




# The Parallel Walled Surgical Kit & Component Assembly

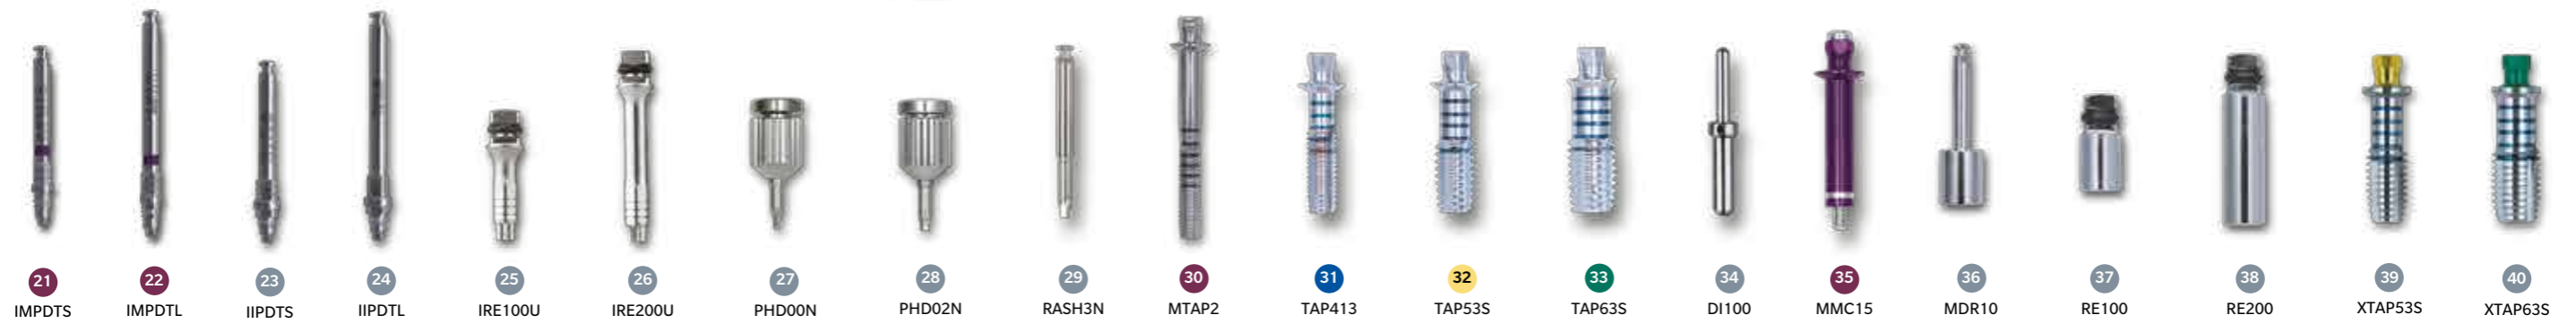

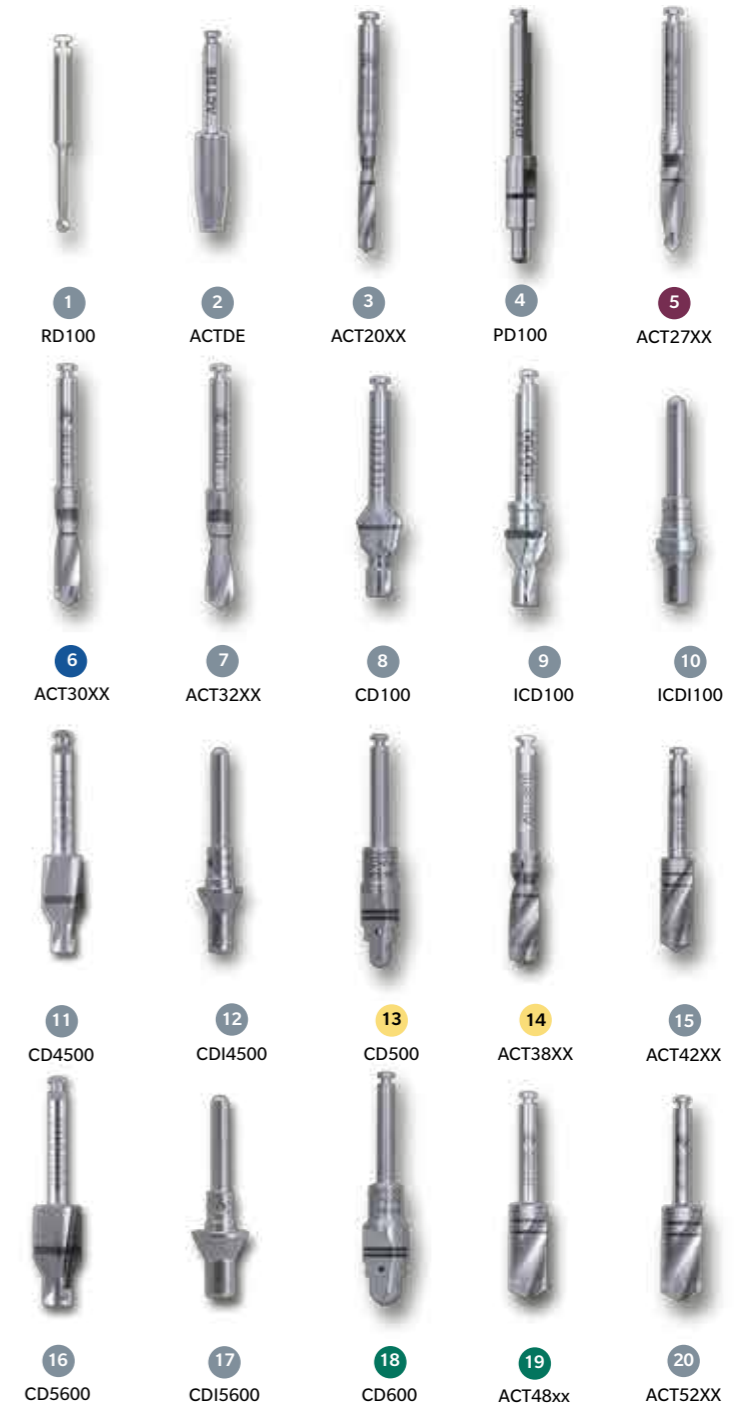


# Simple Steps For The Selection And Replacement Of Instrumentation

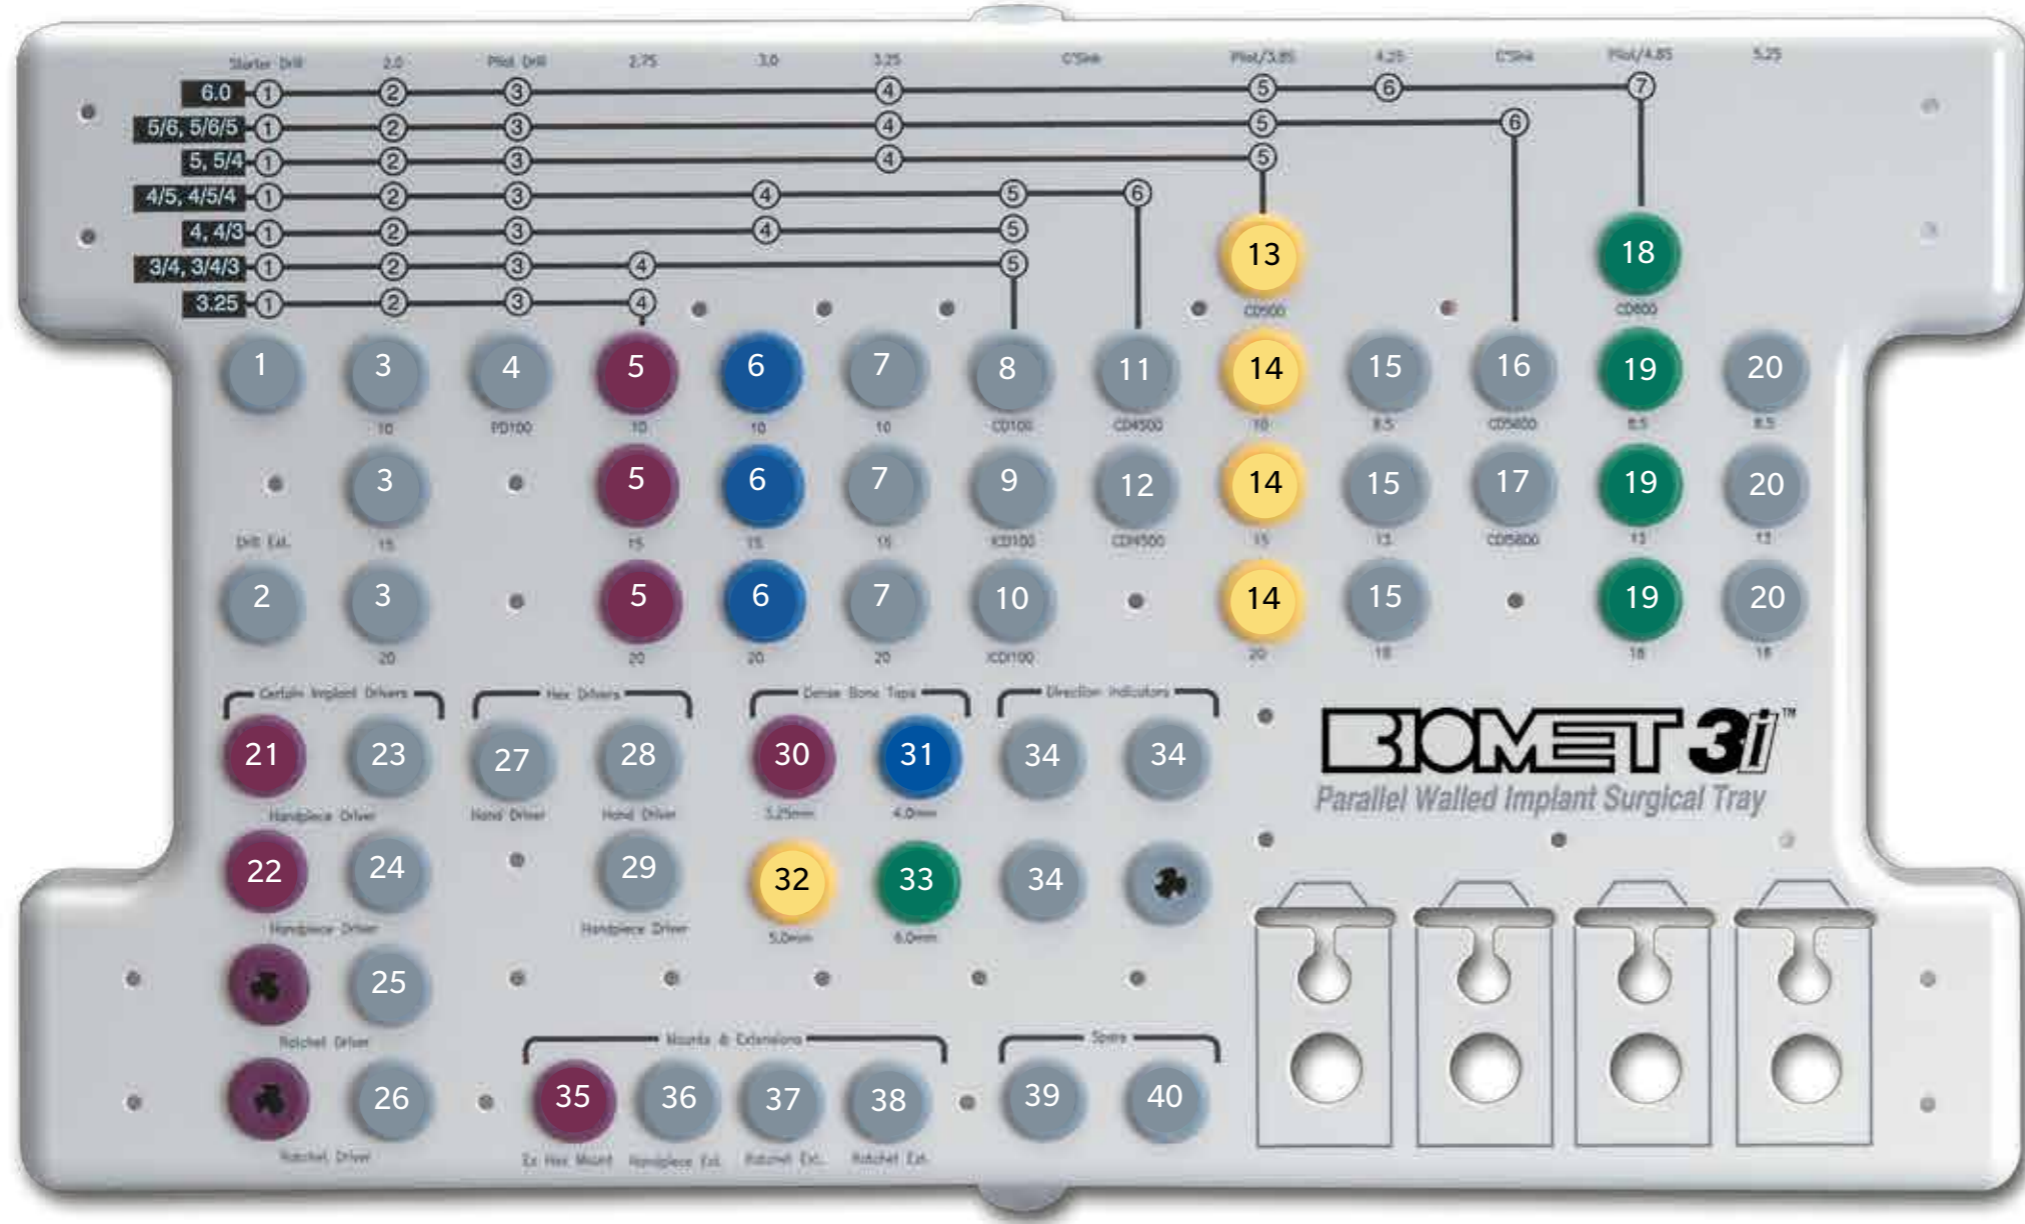










## Parallel Walled Surgical Kits

 PSKT01 Starter (Basic) Kit	 PSKT35 Certain® Premium Kit	 PSKT40 Premium Kit	Description	Item Numbers
•	•	•	Plastic Surgical Tray Organizer	PTT300I
		•	Plastic Tray Organizer for PTT300I	PTT100
	•	•	ACT® Reusable Twist Drill, 2 mm(D) x 10 mm(L)	ACT2010
•	•	•	ACT Reusable Twist Drill, 2 mm(D) x 15 mm(L)	ACT2015
	•	•	ACT Reusable Twist Drill, 2 mm(D) x 20 mm(L)	ACT2020
	•	•	ACT Reusable Twist Drill, 2.75 mm(D) x 10 mm(L)	ACT2710
•	•	•	ACT Reusable Twist Drill, 2.75 mm(D) x 15 mm(L)	ACT2715
		•	ACT Reusable Twist Drill, 2.75 mm(D) x 20 mm(L)	ACT2720
	•	•	ACT Reusable Twist Drill, 3 mm(D) x 10 mm(L)	ACT3010
•	•	•	ACT Reusable Twist Drill, 3 mm(D) x 15 mm(L)	ACT3015
		•	ACT Reusable Twist Drill, 3 mm(D) x 20 mm(L)	ACT3020
	•	•	ACT Reusable Twist Drill, 3.25 mm(D) x 10 mm(L)	ACT3210
•	•	•	ACT Reusable Twist Drill, 3.25 mm(D) x 15 mm(L)	ACT3215
		•	ACT Reusable Twist Drill, 3.25 mm(D) x 20 mm(L)	ACT3220
	•	•	ACT Reusable Twist Drill, 3.85 mm(D) x 10 mm(L)	ACT3810
•	•	•	ACT Reusable Twist Drill, 3.85 mm(D) x 15 mm(L)	ACT3815
	•	•	ACT Reusable Twist Drill, 3.85 mm(D) x 20 mm(L)	ACT3820
	•	•	ACT Reusable Twist Drill, 4.25 mm(D) x 8.5 mm(L)	ACT4285
•	•	•	ACT Reusable Twist Drill, 4.25 mm(D) x 13 mm(L)	ACT4213
	•	•	ACT Reusable Twist Drill, 4.25 mm(D) x 18 mm(L)	ACT4218
	•	•	ACT Reusable Twist Drill, 4.85 mm(D) x 8.5 mm(L)	ACT4885
	•	•	ACT Reusable Twist Drill, 4.85 mm(D) x 13 mm(L)	ACT4813
	•	•	ACT Reusable Twist Drill, 4.85 mm(D) x 18 mm(L)	ACT4818
	•	•	ACT Reusable Twist Drill, 5.25 mm(D) x 8.5 mm(L)	ACT5285
	•	•	ACT Reusable Twist Drill, 5.25 mm(D) x 13 mm(L)	ACT5213
	•	•	ACT Reusable Twist Drill, 5.25 mm(D) x 18 mm(L)	ACT5218
•	•	•	ACT Drill Extension	ACTDE
	•	•	Countersink Drill, Osseotite XP® 4mm/5mm, Prevail® 4/5/4	CD4500
	•	•	Countersink Depth Indicator for CD4500	CDI4500
•	•	•	Countersink/Pilot Drill, 5 mm(D) Implant	CD500
	•	•	Countersink Drill, Osseotite XP 5mm/6mm, Prevail 5/6/5	CD5600
	•	•	Countersink Depth Indicator for CD5600	CDI5600
•	•	•	Certain Countersink Drill, 4 mm(D) Implant	ICD100





### Parallel Walled Surgical Kits



 PSKT01 Starter (Basic) Kit	 PSKT35 Certain® Premium Kit	 PSKT40 Premium Kit	Description	Item Numbers
•	•	•	Countersink Depth Indicator for ICD100	ICD100
•		•	Countersink Drill, 4.1 mm	CD100
	•	•	Countersink/Pilot Drill, 6 mm(D)	CD600
•	•	•	Pilot Drill, 2-3 mm(D)	PD100
•	•		Implant Dense Bone Tap, 3.25 mm(D) x 18 mm(L)	MTAP2
	•	•	Implant Dense Bone Tap, 4 mm(D) x 13 mm(L)	TAP413
	•	•	Implant Dense Bone Tap, 5 mm(D) x 13 mm(L)	TAP53S
		•	Implant Dense Bone Tap, 6 mm(D) x 13 mm(L)	TAP63S
	•	•	Osseotite 2 Dense Bone Tap, 5 mm(D) x 7-13 mm(L)	XTAP53S
		•	Osseotite 2 Dense Bone Tap, 6 mm(D) x 7-13 mm(L)	XTAP63S
	•	•	Certain Implant Driver Tip (Short), 3.4 mm(D)	IMPDTS
•	•	•	Certain Implant Driver Tip (Long), 3.4 mm(D)	IMPDTL
•	•	•	Certain Implant Placement Driver Tip (Short), 4.1, 5, 6 mm(D)	IIPDTS
•	•	•	Certain Implant Placement Driver Tip (Long), 4.1, 5, 6 mm(D)	IIPDTL
•	•	•	Certain Universal Ratchet Extension Driver (Short), 6 mm(L)	IRE100U
•	•	•	Certain Universal Ratchet Extension Driver (Long), 15 mm(L)	IRE200U
•		•	Narrow Small Hex Hand Driver, 17 mm(L)	PHD00N
•	•	•	Narrow Large Hex Hand Driver, 17 mm(L)	PHD02N
•	•	•	Narrow Large Hex Driver, Tip 24 mm(L)	RASH3N
	•	•	Driver Tip Replacement O-Rings, 10-Pack	IRORDR
•	•	•	Handpiece Connector	MDR10
•		•	Open End Wrench	CW100
•	•	•	Ratchet Wrench	WR150
•		•	Ratchet Extension (Short), 6 mm(L)	RE100
•	•	•	Ratchet Extension (Long), 15 mm(L)	RE200
•	•	•	Implant Depth Gauge, 20 mm(L)	DP020
•		•	Implant Mount, 3.4 mm(D) x 15 mm(L)	MMC15
•	•	•	Direction Indicator, 2 mm(D) x 10 mm(L), 3 ea.	DI100
•	•	•	Stainless Steel Round Drill, 2 mm(D)	RD100

## Parallel Walled Surgical Kits

 PSKT10 Starter (Basic) Kit	 PSKT20 Standart Kit	 PSKT30 Premium Kit	 PSKT30U Upgrade Kit	Description	Item Numbers
			•	Plastic Insert for Tray	PTT300UI
•	•	•		Plastic Surgical Tray Organizer	PTT300I
	•	•		Plastic Organizer Tray for PTT300I	PTT100
	•	•		ACT Reusable Twist Drill, 2 mm(D) x 10 mm(L)	ACT2010
	•	•		ACT Reusable Twist Drill, 2 mm(D) x 15 mm(L)	ACT2015
	•	•		ACT Reusable Twist Drill, 2 mm(D) x 20 mm(L)	ACT2020
	•	•		ACT Reusable Twist Drill, 2.75 mm(D) x 10 mm(L)	ACT2710
	•	•		ACT Reusable Twist Drill, 2.75 mm(D) x 15 mm(L)	ACT2715
	•	•		ACT Reusable Twist Drill, 2.75 mm(D) x 20 mm(L)	ACT2720
	•	•		ACT Reusable Twist Drill, 3 mm(D) x 10 mm(L)	ACT3010
	•	•		ACT Reusable Twist Drill, 3 mm(D) x 15 mm(L)	ACT3015
	•	•		ACT Reusable Twist Drill, 3 mm(D) x 20 mm(L)	ACT3020
	•	•		ACT Reusable Twist Drill, 3.25 mm(D) x 10 mm(L)	ACT3210
	•	•		ACT Reusable Twist Drill, 3.25 mm(D) x 15 mm(L)	ACT3215
	•	•		ACT Reusable Twist Drill, 3.25 mm(D) x 20 mm(L)	ACT3220
		•		ACT Reusable Twist Drill, 4.25 mm(D) x 8.5 mm(L)	ACT4285
		•		ACT Reusable Twist Drill, 4.25 mm(D) x 13 mm(L)	ACT4213
		•		ACT Reusable Twist Drill, 4.25 mm(D) x 18 mm(L)	ACT4218
		•		ACT Reusable Twist Drill, 5.25 mm(D) x 8.5 mm(L)	ACT5285
		•		ACT Reusable Twist Drill, 5.25 mm(D) x 13 mm(L)	ACT5213
		•		ACT Reusable Twist Drill, 5.25 mm(D) x 18 mm(L)	ACT5218
	•	•		ACT Drill Extension	ACTDE
	•	•		Pilot Drill, 2-3 mm(D)	PD100
	•	•		Countersink Drill, 4.1 mm	CD100
			•	Certain Countersink Drill, 4 mm(D) Implant	ICD100
		•		Countersink Drill, Osseotite XP 4/5, Prevail 4/5/4	CD4500
		•		Countersink/Pilot Drill, 5 mm(D) Implant	CD500
		•		Countersink Drill, Osseotite XP 5/6, Prevail 5/6/5	CD5600
		•		Countersink/Pilot Drill, 6 mm(D) Implant	CD600
	•	•		Implant Dense Bone Tap, 3.25 mm(D) x 18 mm(L)	MTAP2
	•	•		Implant Dense Bone Tap, 4 mm(D) x 13 mm(L)	TAP413
		•		Implant Dense Bone Tap, 5 mm(D) x 13 mm(L)	TAP53S
		•		Implant Dense Bone Tap, 6 mm(D) x 13 mm(L)	TAP63S
		•		Osseotite 2 Dense Bone Tap, 5 mm(D) x 7-13 mm(L)	XTAP53S
		•		Osseotite 2 Dense Bone Tap, 6 mm(D) x 7-13 mm(L)	XTAP63S
			•	Certain Implant Driver Tip (Short), 3.4 mm(D)	IMPPTS
			•	Certain Implant Driver Tip (Long), 3.4 mm(D)	IMPDTL

### Parallel Walled Surgical Kits

 PSKT10 Starter (Basic) Kit	 PSKT20 Standart Kit	 PSKT30 Premium Kit	 PSKT30U Upgrade Kit	Description	Item Numbers
			•	Certain Implant Placement Driver Tip (Short), 4.1, 5, 6 mm(D)	IIPDTS
			•	Certain Implant Placement Driver Tip (Long), 4.1, 5, 6 mm(D)	IIPDTL
		•	•	Certain Universal Ratchet Extension Implant Driver (Short), 6 mm(L)	IRE100U
			•	Certain Universal Ratchet Extension Implant Driver (Long), 15 mm(L)	IRE200U
•	•	•		Narrow Small Hexed Hand Driver, 17 mm(L)	PHD00N
•	•	•		Narrow Large Hexed Hand Driver, 17 mm(L)	PHD02N
•	•	•		Narrow Large Hex Driver Tip, 24 mm(L)	RASH3N
			•	Driver Tip Replacement O-Rings, 10-pack	IRORDR
•	•	•		Handpiece Connector	MDR10
•	•	•		Open End Wrench	CW100
•	•	•		Ratchet Wrench	WR150
•	•	•		Ratchet Extension (Short), 6 mm(L)	RE100
•	•	•		Ratchet Extension (Long), 15 mm(L)	RE200
•	•	•		Implant Depth Gauge, 20 mm(L)	DP020
	•	•		Implant Mount, 3.4 mm(D) x 15 mm(L)	MMC15
	•	•		Direction Indicator, 2 mm(D) x 10 mm(L), 3 ea.	DI100
	•	•		Stainless Steel Round Drill, 2 mm(D)	RD100

**Icon Descriptions:** The following icons are used to represent the connection type of the implant system:  Internal  External

## Osseotite 2 Dense Bone Tap Ordering Information

Length	5.0 mm(D)	6.0 mm(D)
6.5/7.0(L) - 8.5 mm(L)	XTAP58S	XTAP68S
6.5/7.0(L) - 13.0 mm(L)	XTAP53S	XTAP63S
6.5/7.0(L) - 18.0 mm(L)	XTAP518S	XTAP618S

**Note:** Tapping in dense bone is required. Exceeding an insertion torque of more than 90 Ncm may deform or strip the driver tip or the implant's internal hex and may possibly delay the surgical procedure.



Contact us at 1-800-342-5454 or visit

[zimmerbiometdental.com](http://zimmerbiometdental.com)

Zimmer Biomet Dental  
Global Headquarters  
4555 Riverside Drive  
Palm Beach Gardens, FL 33410  
Tel: +1-561-776-6700  
Fax: +1-561-776-1272

Unless otherwise indicated, as referenced herein, all trademarks are the property of Zimmer Biomet; and all products are manufactured by one or more of the dental subsidiaries of Zimmer Biomet Holdings, Inc., and distributed and marketed by Zimmer Biomet Dental (and, in the case of distribution and marketing, its authorized marketing partners). For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. This material may not be copied or reprinted without the express written consent of Zimmer Biomet Dental. ZBINST979 REV A 07/17 ©2017 Zimmer Biomet, All rights reserved.

